



User Manual



NFS100

Infrared Forehead Thermometer

NFS100 is included as a medical device on the Australian Register of Therapeutic Goods (ARTG No. 198436).

NFS100 is intended for use as a measuring device for determining the patient's body temperature.



ALWAYS READ THE LABEL AND USER GUIDE, USE ONLY AS DIRECTED.

Keep this user guide for future reference. Always retain your proof of purchase in case of warranty service and register your product on line at AUSTRALIA: www.oricom.com.au
Please visit www.oricom.com.au for the latest copy of the user manual.

Oricom Customer Support: 1300 889 785 or (02) 4574 8888

Contents

| | |
|-------------------------------|----|
| Warnings..... | 3 |
| Principle of Measurement..... | 5 |
| Temperature Ranges | 6 |
| Product Descriptions | 7 |
| How to Use NFS100..... | 8 |
| Memory Feature | 9 |
| Mode Change (°C ↔ °F)..... | 10 |
| Battery Replacement..... | 10 |
| Probe Replacement..... | 11 |
| Cleaning Storage | 12 |
| Indications of Errors | 13 |
| Product Specifications..... | 14 |
| Customer Support..... | 15 |
| Warranty information | 16 |



Need Help?

If you need assistance setting up or using your Oricom product now or in the future, call Oricom Support.

Australia 1300 889 785 or (02) 4574 8888
www.oricom.com.au
Mon-Fri 8am – 6pm AEST

New Zealand 0800 67 42 66
www.oricom.co.nz
Mon-Fri 10am – 8pm NZST


Thank you for purchasing the Oricom NFS100 Infrared Forehead Thermometer. The NFS100 is an innovative thermometer using highly developed infrared technology enabling clinical accuracy.

This new type of thermometer enables the user to measure temperature by gently moving the sensor across the forehead.



To use this device correctly please follow the directions in this user guide.

The instructions provide important details on how to achieve accurate measurements.

Warnings



Please read this user guide carefully before initial use and follow all instructions.

- 
- Use this product only for its intended purpose as described in this manual and follow all instructions.
 - The measurement of temperature using this product does not represent a Doctor's medical examination.
 - Consult with your medical professional if any abnormality is found.
 - Do not take a temperature measurement over a scar or open tissue.
 - Do not expose the product to temperatures below 20°C (68°F) or above 50°C (122°F) or a relative humidity of 95% or greater.
 - Do not drop the thermometer as it may cause damage.
 - Do not take temperature with this product near heat sources such as in direct sunlight, near a fireplace or stove.
 - Do not use this product if it is not working properly, contact Oricom support.
 - There are no user serviceable parts the only service required is battery replacement and general cleaning please follow instructions in this user guide.
 - If the product is not going to be used for an extended period of time please remove the battery and store the thermometer in a cool dry place.
- 

- This product is NOT waterproof. Direct contact with water or other liquids should be avoided.
- Do not leave the thermometer with infants or children at any time.
- The protective glass over the lens is fragile, handle with care.
- Do not touch the glass of the infrared lens with bare fingers.


Warning


Many people may not have an elevated temperature even if they are ill. In the following cases please consult your medical professional before using this product.

- Under 90-day-old infants
- People on steroids, antibiotics or antipyretics.
- People with compromised immune systems.

Cautions

- If your child is moving during the measurement it may result in an inaccurate measurement due to the probe losing contact with the skin please calm your child and try again.
- In forehead measurement, slowly move the product from starting point to end for 3 seconds.
- The reliability of the measurement cannot be guaranteed if the temperature is measured from parts of body that are not recommended (anywhere other than the forehead or behind the earlobe).
- Wait 30 seconds between repeat measurements.
- Similar to other thermometer, measurement error may occur within a range of $\pm 0.2^{\circ}\text{C}$ ($\pm 0.4^{\circ}\text{F}$).
- Measurement should not be taken until completely relaxed at normal room temperature.



- Please note that measurement may be incorrect after exercising, bathing or getting wet in the rain.
- For accurate measurement, make sure forehead is clean and free from makeup.
- Temperature between right and left forehead could be different. Always take the temperature from the same side of the forehead.
- Measurement may be incorrect when low battery() signal is indicated. Replace the battery and re-measure.
- When measuring the temperature of a liquid (milk, water) place the probe as close as possible to the liquid but ensure that it is not immersed into the liquid as this may damage your thermometer.

Principle Of Measurement

According to Clinical studies the temperature of the blood in a major artery will reflect an accurate body temperature.

This Infrared Forehead Thermometer is designed to measure the temperature of the skin over the temporal artery, a major artery of the forehead.

The NFS100 is easy and gentle to use it is non-invasive unlike other types of thermometers for measuring rectal, oral underarm and ear areas.

NFS100 ensures faster and easier measurement with a degree of clinical accuracy and several user-friendly functions.

Temperature Ranges

Body temperature means internal temperature of body. Normal temperature even in a healthy person can vary within a small range. The temperature of a person measured in the evening is normally 0.5°C higher than early morning and is also affected by the environment, time and activity. Refer to the table below to find out the normal body temperature ranges.

Normal temperature range at various parts of body

| | |
|--------|--------------------------------|
| Armpit | 34.7 ~ 37.3°C (94.5 ~ 99.1°F) |
| Mouth | 35.5 ~ 37.5°C (95.9 ~ 99.5°F) |
| Rectum | 36.6 ~ 38.0°C (97.9 ~ 100.4°F) |
| Ear | 35.8 ~ 38.0°C (96.4 ~ 100.4°F) |

Normal temperature range by age


| | |
|-------------|--------------------------------|
| 0 ~ 2age | 36.4 ~ 38.0°C (94.5 ~ 100.4°F) |
| 3 ~ 10age | 36.1 ~ 37.8°C (97.0 ~ 100.0°F) |
| 11 ~ 65age | 35.9 ~ 37.6°C (96.6 ~ 99.7°F) |
| Above 65age | 35.8 ~ 37.5°C (96.4 ~ 99.5°F) |

- Normal body temperature can vary between individuals it is recommended that you record your body temperature when you are healthy as a reference point.



NFS100

Product Descriptions

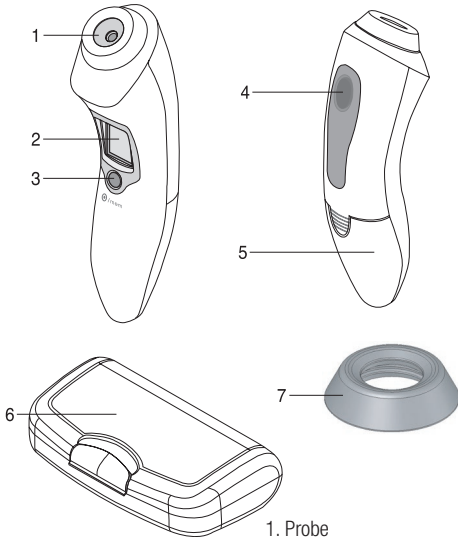


1. Probe
2. LCD Display
3. Power/Memory Button
4. Scan Button
5. Battery Cover
6. Carrying Case
7. Spare Probe

How to Use NFS100



1. Press /mem button as illustrated.



2. All symbols are displayed on LCD when started.



3. When ready symbol (- - -) shows on the display, thermometer is ready to use.



4. Gently hold the NFS100 as illustrated. Press and hold the scan button then place the probe flat and firmly on the skin.



5. Slowly slide the probe midline across the forehead to the hairline keeping the instrument flat and in contact with skin. You should scan the forehead slowly, just like wiping the skin, for 3 seconds and then release the scan button. Measurement should start from center of the forehead.



(O) (X)



6. The unit beeps one time (1) per second, the final beep only occurs after the scan button is released, the thermometer should remain in contact with the skin once the scan button is released until the final beep is heard.

7. Read the temperature on display.
8. As per cautionary notices on pages 4-5 you should allow 30 seconds between each new measurement.
9. The thermometer will automatically turn off after one minute of no-use.

[NOTE]

- Follow instructions 1 to 4 and 6 replace only instruction 5 with instruction below.
- Normally, the artery behind the earlobe does not provide a sufficiently accurate reading. However, in this case due to the effect of sweat lowering the temperature, taking the temperature behind the earlobe may give a better result.
- Brush hair aside if covering the ear and wait for 30 seconds for more accurate measurement. Then gently nestle the NFS100 on neck directly behind earlobe and scan through the arrow direction about 1~2cm (0.4~0.8inch) as illustrated for 3 seconds.
- You should slide the product until you hear a “beep” sound, which indicates the end of the measurement, and then release it from skin.

Memory Feature

NFS100 stores the last 8 readings

Last measured data is automatically stored in order to review the stored temperature.

Pressing \odot /mem will show MEM 1



Pressing \odot /mem again will show MEM 2




Pressing \odot / mem third time will show MEM 3




Memory location with no data will not be displayed.




Pressing and holding /mem for 5 seconds deletes the memory.




Mode Change (°C ↔ °F)

To change from °C to °F press and hold the mem/, and scan button at the same time for 2 seconds.

Battery Replacement

This product contains one lithium battery. When low battery indication () is displayed on LCD, replace the battery as follows:




To remove the battery cover. Press and slide the battery door as indicated by the arrow in the illustration. To replace the battery. Using a pen or similar probe press latch to release the battery.



Place the new battery with the "+" mark facing up. Replace the battery door cover.



Don't throw used lithium batteries in the bin. Keep them safely out of reach of children before disposing them. Ask your local council for the nearest location to dispose your batteries safely.



WARNINGS:

Make sure there are no loose batteries within any child's reach. If you're changing a button battery, do it on a surface out of reach of children.

Make sure the battery cover is secure so your child can't remove it.

Store button batteries like you would any medication – out of reach of children.

If you're suspicious that your child has swallowed a button battery, or has placed one in his/her nose, seek medical attention immediately. Do not give any food or water.

If you find the battery has leaked fluid please do not touch the battery or fluid.


Dispose of the battery properly do not wrap in metal or aluminum foil, wrap in newspaper and dispose of carefully. Battery may explode if burnt or exposed to excessive heat. Check your product regularly for damage and exhausted battery.

Probe Replacement

An additional probe is supplied with your product. If the probe is contaminated or probe surface is damaged, please replace the probe. Turn the probe counter-clockwise to remove. As the probe is a consumable item please contact Oricom if you need to purchase additional probes.

WARNING:

Keep probes out of reach of children.









Cleaning and Storage



- The sensor is a very sensitive part and easily damaged. For accurate measurement please keep the sensor clean.
 - To clean the sensor please keep it facing down and carefully clean with an alcohol moistened cotton bud, allow to dry for at least one hour before using.
 - To clean the outside of the probe use a cloth moistened with alcohol or water.
 - Do not use excessive force on the sensor.
- Do not immerse the product in water or any other liquid.
 - Keep the product away from direct sunlight, dust and any other type of contaminating substance.
 - Keep the product at normal room temperature. The operating ambient temperature range for this thermometer is 16°C (60.8°F) to 40°C (104°F)
 - Please place the product in normal room temperature for 30 minutes prior to use if it has been stored outside normal room temperature.

Indications Of Errors

| | |
|--|---|
|  | <p>Q: Outside temperature is below 10°C (50°F) or above 40°C (104°F) A: Place the product where temperature is between 10°C (50 °F) and 40°C (104°F) for 30 minutes.</p> |
|  | <p>Q: Measured object is above 42.2°C (108°F) A: Recheck the measured object before measuring. (Extremely hot object cannot be measured)</p> |
|  | <p>Q: Measured object is below 20°C (68°F) A: Recheck the measured object before measuring. (Extremely cold object cannot be measured)</p> |
|  | <p>Q: System Error A1: Turn off for 1 minute and turn on again A2: remove and replace the battery turn on again A3: Consult Oricom support</p> |
|  | <p>Q: Informing battery replacement time A: Replace the battery</p> |
|  | <p>Q: Informing inactivity due to low battery A: Replace the battery</p> |
| Inaccurate measurement | <p>Q: After bathing or returning home A: Need time to relax. Q: Measured value is different. A: Probe and forehead must be at right angles to each other.</p> |
| 3 Short "beep" Sounds | <p>Q: Low battery indication, system error or mal - function. A: remove and replace the battery then turn power on again.</p> |

Product Specifications

| Items | Descriptions |
|--------------------|---|
| Measurement Method | Infrared measurement |
| Measuring Time | 3 sec for forehead |
| Temperature | 20(68.4) ~ 42.2°C (108.0°F) |
| Measurement Range | |
| Accuracy | ±0.2°C (±0.4°F) : 20 ~ 42.2°C (68.4 ~ 108.0°F) |
| Display Type | LCD (Liquid Crystal Display) |
| Memory Capacity | 8 readings |
| Power Save Mode | Automatic shutdown after 1 minute of non-use |
| Battery | CR2032 (1ea.) About 6,000 readings |
| Dimensions | 33mm(W) X 42mm(D) X 143mm(H) |
| Weight | 60g(2.1oz) with battery |
| Ambient Conditions | 16~40°C (60.8~104°F), Humidity : below 95% Atmospheric Pressure(hPa) 700~1060 |
| Transport | -20~50°C (59~104°F), Humidity : below 95% |
| Storage condition | Atmospheric Pressure(hPa) 700~1060 |




Type BF Applied Parts

NFS100 is included as a medical device on the Australian Register of Therapeutic Goods (ARTG No. 198436).

NFS100 is intended for use as a measuring device for determining the patient's body temperature. ALWAYS READ THE LABEL AND USER GUIDE, USE ONLY AS DIRECTED.

This product is manufactured in Korea under strict quality supervision by: HuBDIC CO., Ltd, B-301, TaeKwang Industrial Building, 191-1, Anyang 7-dong Manan-gu, Anyang-si Gyeonggi-do Korea.
IMPORTED & DISTRIBUTED IN AUSTRALIA by the sponsor:- Oricom International Pty Ltd, Unit 1, 4 Sovereign Place, South Windsor 2756 AUSTRALIA






Customer Support

If you have any problems setting up or using this product you will find useful tips and information in this user guide as well as “Frequently Asked Questions” on our website www.oricom.com.au.

If you have further questions about using the product after reviewing the resources above or would like to purchase replacement parts or accessories please call our Customer Support Team. Our dedicated local support team are more likely to be able to help you than the retailer where you made your purchase.

Important

Please retain your purchase receipt and attach to the back page of this user guide as you will need to produce this if warranty service is required. Take a few moments to register your product online: www.oricom.com.au



Express Warranty (Australia)

This Express Warranty is provided by Oricom International Pty Ltd ABN 46 086 116 369, Unit 1, 4 Sovereign Place, South Windsor NSW 2756, herein after referred to as “Oricom”.


Oricom products come with guarantees that cannot be excluded under the Australian Consumer Law. You are entitled to a replacement or refund for a major failure and compensation for any other reasonably foreseeable loss or damage. You are also entitled to have the goods repaired or replaced if the goods fail to be of acceptable quality and the failure does not amount to a major failure.

Oricom warrants that the product is free from defects in materials or workmanship during the Express Warranty Period. This Express Warranty does not extend to any product from which the serial number has been removed or was purchased outside of Australia.

Nothing in this Express Warranty excludes, restricts or modifies any condition, warranty, guarantee, implied term, right or remedy pursuant to the Australian Consumer Law and which may not be so excluded, restricted or modified. For such conditions, terms, guarantees and warranties that cannot be excluded, restricted or modified, Oricom limits the remedies available to extent permitted in the relevant legislation.

The Express Warranty Period will be 1 year from the date of purchase of the product evidenced by your dated sales receipt. You are required to provide proof of purchase as a condition of receiving Express Warranty services.

You are entitled to a replacement product or repair of the product at our discretion according to the terms and conditions of this document if your product is found to be faulty within the Express Warranty Period. This Express Warranty extends to the original purchaser only and is not transferable.




Products distributed by Oricom are manufactured using new materials or new and used materials equivalent to new in performance and reliability. Spare parts may be new or equivalent to new. Spare parts are warranted to be free from defects in material or workmanship for thirty (30) days or for the remainder of the Express Warranty Period of the Oricom branded product in which they are installed, whichever is longer. During the Express Warranty Period, Oricom will where possible repair and if not replace the faulty product or part thereof. All component parts removed under this Express Warranty become the property of Oricom. In the unlikely event that your Oricom product has a recurring failure, Oricom may always, subject to the Competition and Consumer Act 2010, at its discretion, elect to provide you with a replacement product of its choosing that is at least equivalent to your product in performance.

No change to the conditions of this Express Warranty is valid unless it is made in writing and signed by an authorised representative of Oricom.

Oricom will not be liable under this Express Warranty, and to the extent permitted by law will not be liable for any defect, loss, damage or injury arising out of or in connection with a:

1. failure by you to adhere to the warnings and follow the instructions set out in this user guide for the proper installation and use of the product;
2. wilful misconduct or deliberate misuse by you of the product;
3. any external cause beyond our control, including but not limited to power failure, lightning or over voltage; or
4. modification to the product or services carried out on the product by anyone other than Oricom or Oricom's authorised service provider.



How to make a claim under your Express Warranty in Australia

Oricom has a simple warranty process for you to follow:

- Please call or email our Customer Support Team, 1300 889 785 or support@oricom.com.au.
- A Customer Support Team member will verify after troubleshooting with you if your product qualifies under warranty. If so, they will give you a Product Return Authorisation number.
- We will then email or fax a Return Authorisation form and a Repair Notice (if necessary), together with instructions on how to return the goods for warranty service.


Please note that if a Customer Support Team member advises that your product does not qualify for return, this warranty does not apply to your product. Products that are authorised to be returned to Oricom in Australia must include all of the following:

- A completed Return Authorisation form
- A copy of your Proof of Purchase (please keep your original copy)
- The faulty product, including all accessories.

Send the approved returns to:

Oricom International Pty Ltd
Locked Bag 658
South Windsor NSW 2756 Australia

Please note that this Express Warranty excludes expenses incurred by you in returning any faulty product to us. You must arrange and pay any expenses incurred (including postage, delivery, freight, transportation or insurance of the product) to return the faulty product to us, however, we will arrange delivery of the repaired or replaced faulty product to you.






NFS100

Important Information

Repair Notice

Please be aware that the repair of your goods may result in the loss of any user-generated data (such as stored telephone numbers, text messages and contact information). Please ensure that you have made a copy of any data saved on your goods before sending for repair. Please also be aware that goods presented for repair may be replaced by refurbished goods or parts of the same type rather than being repaired.





Contact details for Oricom Support and Express Warranty Claims in Australia

Oricom International Pty Ltd
Locked Bag 658
South Windsor, NSW 2756
Australia

Email: support@oricom.com.au
Phone: 1300 889 785 or (02) 4574 8888
(Monday to Friday 8am to 6pm AEST)
Web: www.oricom.com.au
Fax: (02) 4574 8898

Contact details for Oricom Support and Express Warranty Claims in New Zealand

Email: support@oricom.co.nz
Phone: 0800 674 266
(Monday to Friday 10am to 8pm NZST)
Web: www.oricom.co.nz

Ref: 21012015